



KB03004
Lowry Protein
Quantification
Assay Kit

1200 tests (96 well plate)/
48 tests (test tube)

Votre interlocuteur en France, Belgique, Luxembourg et Suisse :
LIBIOS

83, rue Edmond Michelet - 69490 Pontcharra Sur Turdine - France
Tél. : +33 (0)4 74 13 03 02 - Fax : +33 (0)4 74 05 28 25 –
Mail : info@libios.fr - www.libios.fr

Table of contents

1.	General information	1
2.	Technical specifications	2
3.	Materials and storage	3
4.	Introduction	4
5.	Assay principle	4
6.	Assay preparation	5
7.	Sample preparation	7
8.	Assay protocol	8
9.	Data analysis	10
10.	Troubleshooting	12
11.	Additional information	14
12.	Related products	14
13.	Warranties and limitation of liability	15

1. General information

PRECAUTIONS

Please read this manual carefully before beginning the assay.

This product is designed for **research use only**. It is not approved for human or animal use or clinical diagnosis. All chemicals should be handled with care and in accordance with laboratory safety practices. It is recommended to use basic Personal Protective Equipment.

Do not use after the expiration date stated on the packaging.

Do not mix or substitute reagents or materials from other kit batches or vendors.

For the **material safety data sheet** (MSDS) please contact us at info@bioquochem.com

TECHNICAL RECOMMENDATIONS

Store reagents as indicated in **Materials and storage** section.

Be sure to keep the bottle capped when not in use.

Let the components reach room temperature (RT) before use.

Immediately before use, gently invert and rotate reagent bottles several times to mix the contents thoroughly.

Avoid foaming or bubbles when mixing or reconstituting components.

Avoid cross contamination of samples or reagents by changing pipette tips between sample, standard and reagent additions.

Be sure to use the optimal microplate for the assay. Flat bottom, transparent microplates for UV/VIS applications, and black microplates for fluorescence measurements.

2. Technical specifications

Available sizes

Test tube format: 48 tests

Microplate format: 1200 tests

Required sample volume

Test tube format: 1 mL/test

Microplate format: 40 μ L/test

Compatible samples

Biological fluids, food, and beverages

Type of detection

Colorimetric (660 nm)

3. Materials and storage

MATERIALS SUPPLIED

Item	Units	Storage
Reagent A	4	RT
Reagent B	2	RT
Reagent C	1	RT
Protein Standard	1	4 °C
Transparent 96-Well Microplate	2	RT

MATERIALS NEEDED BUT NOT SUPPLIED

- Double distilled water (ddH₂O) as Milli-Q Ultrapure Water
- Labware materials (micropipettes, tubes, stirring/mixing equipment)
- Colorimetric microplate reader – equipped with filter for OD 660 nm

STORAGE CONDITIONS

On receipt, store kit components as indicated above. Under these conditions, the reagents are stable in the original packaging until the expiration date indicated on the outside of the box. After reconstitution, protein standard solution should be stored at -20 °C. Prepare a fresh set of standards for every use.

4. Introduction

The Lowry Protein Assay is a biochemical assay for determining the total level of protein in a solution, first described in 1951. This method has been the most widely used assay to estimate the amount of proteins in biological samples due to its sensitivity, simplicity, and precision.


Proteins are biopolymeric structures composed of amino acids that play many critical roles in the body. Protein is also a vital part of the human diet. Protein quantification assays are therefore fundamental to biological research, clinical diagnosis or food industry.

The Lowry Assay is relatively sensitive but requires more time than other assays and is susceptible to many interfering compounds.

BQC Lowry Protein Quantification Assay Kit is a simple test for the quantification of proteins in in different type of samples.

5. Assay principle

BQC Lowry Protein Quantification Assay Kit is based on the Lowry method. This method relies on two chemical reactions. The first is the Biuret reaction, in which protein reacts with cupric sulfate and tartrate in an alkaline solution, resulting in formation of copper-protein complexes. The second reaction is the reduction of the Folin-Ciocalteu Reagent (phosphomolybdate and phosphotungstate) by the previously formed chelated copper complexes producing a colored product that can be measured at 660 nm. The protein concentration in a sample is determined from a calibration curve using bovine serum albumin (BSA) as standard.

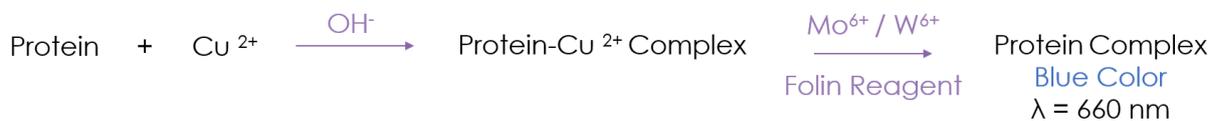

Principle of the Lowry Protein Assay Kit

6. Assay preparation

REAGENT PREPARATION

All assay reagents not listed below are ready to use as supplied. Allow the reagents to reach room temperature before use.

- ⚠ **CAUTION:** Before preparing **Lowry Assay Mix** and **Lowry Working Solution** consider the number of tests to be performed. Both solutions must be prepared fresh daily

Lowry Assay Mix: Mix Reagent B with Reagent A in a 1:100 ratio to prepare the desired volume.

Lowry Working Solution: Dilute Reagent C with an equal volume of ddH₂O (1:1 ratio) to prepare the desired volume.

Protein Standard Solution (Bovine Serum Albumin, BSA): Add 3 mL of ddH₂O to the Standard vial. Mix carefully to avoid foaming.

- ⚠ **NOTE:** Aliquot and store at -20 °C the Standard Solution for long term use

STANDARD CALIBRATION

Test tube Lowry Protein Quantification

Prepare BSA standards for the calibration curve from the Standard solution according to the following Table. Prepare the standards immediately prior to each assay. Mix carefully to avoid foaming.

Standard	Standard solution (µL)	*Diluent (µL)	Protein (µg/mL)
Std 1 (Reagent Blank)	0	2000	0
Std 2	10	1990	50
Std 3	30	1970	150
Std 4	60	1940	300
Std 5	100	1900	500
Std 6	160	1840	800

*Use as diluent the buffer used in the samples

Microplate Lowry Protein Quantification

Prepare BSA standards for the calibration curve from the Standard solution according to the following Table. Prepare the standards immediately prior to each assay. Mix carefully to avoid foaming.

Standard	Standard solution (μL)	*Diluent (μL)	Protein (μg/mL)
Std 1 (Reagent Blank)	0	500	0
Std 2	2.5	497.5	50
Std 3	7.5	492.5	150
Std 4	15.0	485.0	300
Std 5	25.0	475.0	500
Std 6	40.0	460.0	800

*Use as diluent the buffer used in the samples

BQC recommends running the standards and samples at least in duplicate (triplicate recommended). There is no specific pattern for using the wells on the plate. A proposed layout of standards (Std) and samples (S) to be measured in duplicate is shown below.

NOTE: If sample blanks are included in the assay, it is necessary to reserve some wells of the plate for these blanks

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 1	Std 1	S3	S3	S11	S11	S19	S19	S27	S27	S35	S35
B	Std 2	Std 2	S4	S4	S12	S12	S20	S20	S28	S28	S36	S36
C	Std 3	Std 3	S5	S5	S13	S13	S21	S21	S29	S29	S37	S37
D	Std 4	Std 4	S6	S6	S14	S14	S22	S22	S30	S30	S38	S38
E	Std 5	Std 5	S7	S7	S15	S15	S23	S23	S31	S31	S39	S39
F	Std 6	Std 6	S8	S8	S16	S16	S24	S24	S32	S32	S40	S40
G	S1	S1	S9	S9	S17	S17	S25	S25	S33	S33	S41	S41
H	S2	S2	S10	S10	S18	S18	S26	S26	S34	S34	S42	S42

Example of plate layout for the Lowry Protein Quantification Assay Kit

7. Sample preparation

The following sample preparation protocols are intended as a guide only. The optimal conditions for sample preparation must be determined by the end user. It is recommended to use fresh samples. If it is not possible, aliquot and store samples appropriately with minimal freeze/thawing.

Lowry Protein Quantification Assay Kit can be used to determine proteins in a wide variety of samples like biological fluids, food, and beverages.

Reagents and materials required for sample preparation are not supplied with the kit. Before doing sample preparation, consider the volume of sample required per test; see **Technical specifications** section.

Make sure that interfering substances present in the sample do not give a significant background. Run proper blanks as necessary (e.g. sample blank should be always evaluated when working with highly colored samples).

Chelating substances, strong acids or bases, reducing agents, ascorbic acid, uric acid, iron, potassium, tyrosine, etc. have been reported to interfere with the Lowry assay and should be minimized as components of the sample buffer.

Interfering substances can be removed by protein precipitation with acetone or trichloroacetic acid (TCA). Once dissolved, the obtained protein pellet can be used for the assay. It is also possible to remove the interfering substances by dialysis or gel filtration.

It is recommended to assay different sample dilutions to ensure the values fall within the standard curve.

8. Assay protocol


Prepare and mix all reagents thoroughly before use. Each standard, sample or blank should be assayed at least in duplicate.

Test tube Lowry Protein Quantification Kit (6.5 mL)

-  Pipette **1 mL** of **standard** or **sample** into test tubes (not included)
-  Add **5 mL** of **Lowry Assay Mix** to each tube and thoroughly vortex
-  **Incubate** the tubes for **10 minutes** at **RT**
-  Add **0.5 mL** of **Lowry Working Solution** to each tube and vortex immediately
-  **Incubate** the tubes for **30 minutes** at **RT**
-  Vortex the tubes and read the **absorbance** at **660 nm**

Note: The Lowry assay is not an end point assay. Significant changes in the absorbance of a sample are expected if a long time elapses between sample readings (> 10 min).

Microplate Lowry Protein Quantification Kit

-  Set up the plate design
-  Add **40 µL** of **standard** or **sample** in each well
-  Add **200 µL** of **Lowry Assay Mix** in each well and mix by pipetting
-  **Incubate** the microplate for **10 minutes** at **RT**
-  Add **20 µL** of **Lowry Working Solution** in each well and mix by pipetting.
-  **Incubate** the microplate for **30 minutes** at **RT**
-  Read the **absorbance** of all wells at **660 nm** at **RT**


Note: The Lowry assay is not an end point assay. Significant changes in the absorbance of a sample are expected if a long time elapses between sample readings (> 10 min).

If you need to **adapt this kit** for another form of the assay (for example cuvette), **contact us at** info@bioquochem.com

9. Data analysis

ANALYSIS OF THE STANDARDS

- Calculate the average absorbance of the standards.
- Subtract the average absorbance of the reagent blank (Std 1) from the average absorbance of the standards to obtain the blank-corrected absorbance of the standards.
- Create a standard curve by plotting the blank-corrected absorbance of the standards as a function of the standard concentration. A typical standard curve ($y = \text{slope} \cdot x \pm \text{intercept}$) for the microplate assay procedure is shown below.

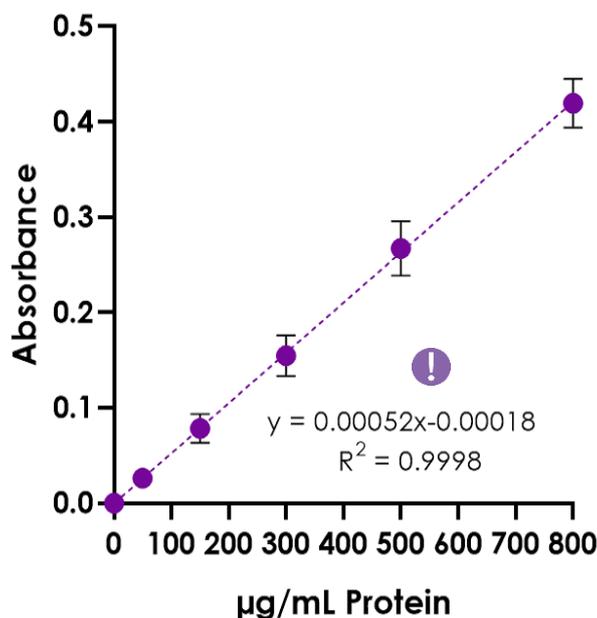

Protein standard curve with Lowry Protein Quantification Assay Kit

- ⓘ This standard curve is an example of the data typically obtained with this kit. **DO NOT USE** this standard curve to calculate the protein concentration of your samples. A new standard curve must be performed by the end user.

ANALYSIS OF THE SAMPLES

- Calculate the average absorbance of the samples.
- Subtract the average absorbance of the reagent blank (Std 1) from the average absorbance of each sample to obtain the blank-corrected absorbance of the samples.
- Calculate the protein concentration of the samples using the following equation. Slope and intercept values are obtained from the standard curve.

$$\text{Protein } (\mu\text{g/mL}) = \left(\frac{A_s - \text{intercept}}{\text{slope}} \right)$$

When working with diluted samples the concentration values obtained must be multiplied by the dilution factor to obtain the protein concentration of the undiluted sample.

10. Troubleshooting

This troubleshooting table provides potential sources and solutions for common problems observed with BQC Assay Kits. **The problems listed below could occur when using any BQC Assay Kit.** They are not specific for this assay kit.

Problem	Possible Cause	Recommended Solution
Wells have color but there is no reading	Plate read at incorrect wavelength	Check the wavelength used in the assay
	Incorrect microplate	Use the correct microplate for your application UV/Vis: transparent Fluorescence: black wells/transparent bottom
Standard readings do not follow a linear pattern	Pipetting errors in preparation of standards	Avoid pipetting small volumes (<5 μ L) Be careful not to splash from well to well
	Air bubbles formed in well(s)	Use reverse pipetting technique
	Standard stock is at incorrect concentration	Always refer to dilutions described in Assay preparation
	Improperly thawed reagents	Thaw all components completely and mix well before use
	Use of improperly stored reagents	Store the components appropriately Use fresh components from the standard curve
	Incorrect incubation times or temperatures	Refer to Assay protocol
Dispersion of standard and sample readings	Pipetting errors	Avoid pipetting small volumes (<5 μ L) Be careful not to splash from well to well
	Air bubbles formed in well(s)	Use reverse pipetting technique

Problem	Possible Cause	Recommended Solution
Sample erratic values	Samples contain interfering substances	Dilute sample further (if possible)
	Inappropriately stored samples or samples used after multiple freeze-thaw cycles	Use fresh samples or store appropriately until use
	Samples not deproteinized	Use an appropriate deproteinization protocol
	Cells/Tissue samples not homogenized completely	Repeat the sample homogenization
	Inappropriate sample dilution buffer	Refer to Assay preparation
Sample reading fall outside the detection range	Samples are too diluted/concentrated No analyte/activity is observed in the sample	Re-assay using different sample dilutions

STILL HAVING PROBLEMS?

Contact BQC if you have any further questions, our team will be pleased to help you:



Phone

+ 34 985 26 92 92



E-mail

info@bioquochem.com



Business hours

Monday-Thursday: 8.30 to 17.00 (CEST)

Friday: 8.00 to 15.00 (CEST)

11. Additional information

Lowry Protein Quantification Assay Kit is a simple, sensitive and precise assay (RSD <10 %) for determining proteins in a wide variety of samples.

Ammonium sulphate, dithioerythritol (DTE) and dithiothreitol (DTT) have been reported to interfere with this assay and must be avoided. Commonly used detergents, some chelating agents, reducing agents, many salts, some sugars, glycine, Tris buffer, compounds with sulfhydryl groups, amino acids and phenol also interfere with the Lowry assay at even low concentrations.

If unexpected results are obtained running your samples, please contact us at info@bioquochem.com

12. Related products

More products available on bioquochem.com

Reference	Product
KB03003	Bradford Protein Quantification Assay Kit
KF01002	ABTS Antioxidant Capacity Assay Kit
KB03002	Lipid Peroxidation Assay Kit

13. Warranties and limitation of liability

BQC shall not in any event be liable for incidental, consequential or special damages of any kind resulting from any use or failure of the products, even if BQC has been advised of the possibility of such damage including, without limitation, liability for loss of use, loss of work in progress, downtime, loss of revenue or profits, failure to realize savings, loss of products of buyer or other use or any liability of buyer to a third party on account of such loss, or for any labor or any other expense, damage or loss occasioned by such product including personal injury or property damage is caused by BQC's gross negligence. Any and all liability of BQC hereunder shall be limited to the amounts paid by the buyer for the product.

Buyer's exclusive remedy and BQC's sole liability hereunder shall be limited to a refund of the purchase price, or the replacement of all material that does not meet our specifications.

Said refund or replacement is conditioned on buyer giving written notice to BQC within 30 days of shipment.

Expiration date: 1 year from the date of fabrication. Expiration date is indicated on the outside of the box.

For further details, please refer to our website [bioquochem.com](https://www.bioquochem.com)



Votre interlocuteur en France, Belgique, Luxembourg et Suisse :
LIBIOS

83, rue Edmond Michelet - 69490 Pontcharra Sur Turdine - France
Tél. : +33 (0)4 74 13 03 02 - Fax : +33 (0)4 74 05 28 25 –
Mail : info@libios.fr - www.libios.fr